

ORIGINAL ARTICLE

Effect of different beverages and polishing techniques on colour stability of CAD/CAM composite restorative materials

Lippo Lassila^a, Mine B. Uctasli^b, Kanae Wada^c, Pekka K. Vallittu^{a,d}, and Sufyan Garoushi^a

^aDepartment of Biomaterials Science and Turku Clinical Biomaterial Center – TCBC, Institute of Dentistry, University of Turku, Finland;

^bDepartment of Restorative Dentistry, Faculty of Dentistry, University of Gazi, Turkey; ^cDepartment of Pediatric Dentistry / Special Needs Dentistry, Tokyo Medical and Dental University TMDU, Tokyo, Japan; ^dWellbeing Services County of South-West Finland, Turku, Finland

ABSTRACT

Objectives: The aim of this article was to compare the colour stability of short fibre-reinforced computer-assisted design/computer-assisted manufacturing (CAD/CAM) composite (SFRC CAD) to commercially available CAD/CAM materials following prolonged immersion in a variety of beverages. Furthermore, the influence of the polishing technique was evaluated.

Materials and methods: A total of 120 rectangular specimens (10 mm length × 14 mm width × 2 mm thickness) were prepared from SFRC CAD, IPS e-max, Cerasmart 270, Celtra Duo, Enamic, and Brilliant Crios. The specimens underwent polishing through either a laboratory polishing machine equipped with 4000-grit silicon carbide paper or chairside polishing using Sof-Lex spiral. Twenty specimens of each tested CAD/CAM material were randomly divided into four groups ($n = 5$) based on the staining solution used in order to evaluate the colour stability of the materials. Group 1: distilled water, Group 2: coffee, Group 3: red wine, Group 4: coke. Using a spectrophotometer, the colour changes (ΔE) of all CAD/CAM materials were assessed at baseline, and after 1 and 12 weeks of staining. Three-way analysis of variance was used to analyse the data ($\alpha = 0.05$).

Results: The staining solution and material type showed a significant influence on the CAD/CAM specimens' colour stability ($p < 0.05$), while polishing method had no significant influence ($p > 0.05$). The average ΔE values for specimens submerged in wine were considerably higher ($p < 0.05$) than those for the other solutions. SFRC CAD, Cerasmart 270, and Enamic displayed the highest ΔE values in wine ($p < 0.05$).

Conclusions: The colour stability of tested SFRC CAD was comparable to other composite-based CAD/CAM materials, while IPS e-max exhibited the highest level of colour stability.

ARTICLE HISTORY

Received 30 January 2024

Accepted 4 April 2024

KEYWORDS

Colour stability; staining, SFRC CAD; e.max; polishing technique



Introduction

Recently, there has been a remarkable increase in patients' expectations and interest in indirect restorations. In response to these growing demands, the adoption of metal-free fixed restorations has become highly accepted, driven by their exceptional biocompatibility, chemical and colour stability, reduced surface roughness, and aesthetic advantages [1]. Simultaneously, the use of computer-assisted design/computer-assisted manufacturing (CAD/CAM) has increased owing to significant technological advancements. The primary benefit of CAD/CAM technology lies in the capacity to use uniform and flawless CAD/CAM blocks for creating aesthetic restorations in a single session [2]. Currently on the market, there are CAD/CAM block materials made of glass ceramics, zirconia, composites, and hybrid ceramics [2, 3].

Due to its mechanical and bonding characteristics, lithium disilicate glass ceramic has been used widely for indirect single unit bonded permanent prostheses. Its flexural strength, fracture resistance, and bond strength to resin composite luting cements

are all improved because of the large number of longitudinal crystals it contains [3]. However, it has been noted that lithium disilicate glass ceramic without proper polishing causes wear to antagonist enamel and is a stiff, brittle material that needs more crystallisation to obtain its maximum strength [4]. Nevertheless, adhesion failure may occur as a result of the high elastic modulus, which tends to concentrate extra stress at the adhesive interface [5]. When it comes to zirconia, scientific investigations conducted in controlled laboratory settings have determined that establishing a strong and durable bond between zirconia and the luting cement can be challenging, potentially compromising its long-term durability [6]. Zirconia, especially translucent modifications, have low fracture toughness which limits use of the material clinically [7].

To achieve a more acceptable stress distribution between restoration and underlying tooth structure, some researchers [8, 9] advocate using materials having an elastic modulus similar to that of dentin. Due to elastic modulus, wear characteristics, colour integration, and malleability in thin layers, composite-

CONTACT Sufyan Garoushi  sufgar@utu.fi  Department of Biomaterials Science, Institute of Dentistry and TCBC, University of Turku, Itäinen Pitkätatu 4 B, FI-20520 Turku, Finland

 Supplemental data for this article can be accessed online at <https://doi.org/10.2340/biid.v11.0002>.

© 2024 The Author(s). Published by MJS Publishing on behalf of Acta Odontologica Scandinavica Society. This is an Open Access article distributed under the terms of the Creative Commons Attribution 4.0 International License (<http://creativecommons.org/licenses/by/4.0/>), allowing third parties to copy and redistribute the material in any medium or format and to remix, transform, and build upon the material, with the condition of proper attribution to the original work.

based CAD/CAM materials have become increasingly common over the past 10 years [10, 11]. Compared to traditional light-cured resin composites, CAD/CAM composites have significantly higher monomer conversion due to the high temperature and pressure during polymerisation, resulting in composites with superior mechanical properties and biocompatibility [2]. Clinical outcome of composite-based CAD/CAM materials is still debatable to some extent, though, as evidence suggests many of their mechanical characteristics can be classified as those of ceramics [12, 13].

The development of discontinuous (short) fibre-reinforced CAD/CAM composite (SFRC CAD) aims at enhancing fracture toughness, which will enhance the mechanical characteristics of these composite-based CAD/CAM materials, and reduce issues that might have a negative impact on their long-term clinical performance [14–16]. SFRC CAD had shown good performance when mechanical, loading, optical, surface, and bonding properties were investigated [13–17]. However, no information is available regarding this material's colour stability following exposure to staining solutions. Therefore, the current study's objective was to assess how well SFRC CAD composite maintained its colour after being exposed to common beverages, in comparison to commercially available ceramic and composite-based CAD/CAM materials. The following are the null hypotheses that this study examined: The type of beverage, immersion time, the CAD/CAM material, and the polishing technique have no impact on the staining of restorations.

Materials and methods

A list of the CAD/CAM materials used in the investigation is given in Table 1. Twenty rectangular specimens (10 mm length × 14 mm width × 2 mm thickness) were cut with a water-cooled, low-speed diamond saw (Struers, Glasgow, Scotland) from each CAD/CAM material. Previous research in the literature served as the basis for calculating the sample size [18, 19].

The specimens underwent polishing by rubbing them with 600-grit silicon carbide abrasive paper while water was flowing. After reaching the desired thickness, the lower surface of the specimen was polished using abrasive paper (1000-grit, 2000-

grit, and 4000-grit FEPA) for 20 s each at 300 rpm, with water cooling, using an automatic grinding machine (Struers Rotopol-11, Copenhagen, Denmark). This polished side is referred to as the 'machine polish' side. The specimens' upper surface was polished using 1000-grit abrasive paper. Afterwards, the surfaces underwent polishing using a 3M™ Sof-Lex™ Diamond Polishing System, specifically utilising a pre-polishing spiral and a diamond-impregnated polishing spiral. Each spiral was polished for 20 s using a slow speed hand piece while being cooled with water. This side was referred to as the hand polish. A single operator was responsible for processing all of the specimens.

To achieve consistency, a digital calliper manufactured by Mitutoyo Corp. (Tokyo, Japan) with a precision of 0.01 mm was used to measure the thickness of each specimen. After the polishing technique, the specimens were immersed in distilled water and kept at a temperature of 37°C for 24 h prior to taking the initial colour measurement.

In order to assess the colour change across four distinct beverages, a total of 20 specimens ($n = 5$ per group) from each CAD/CAM material were randomly allocated into four groups based on the staining solution employed. Group 1 consisted of distilled water with a pH of around 7. Group 2 had Nescafe classic coffee from Nestle, where 3.6 grams of coffee powder was dissolved in 300 millilitres of boiling pure water, resulting in a pH of approximately 5. Group 3 consisted of red wine (Frontera Cabernet Sauvignon, Chile) with a pH of approximately 3.5. Group 4 contained coke from the Coca-Cola Company, and had a pH of approximately 2.5.

The specimens were immersed in containers holding the staining solutions, ensuring that both sides were exposed to the solutions. In order to prevent the evaporation of staining solutions, the specimens were kept in sealed containers for the whole course of the investigation. The stained beverages were renewed on a weekly basis. The specimens were kept in an incubator at 37°C all the time, except for when colour measurements and solution changes were made.

The colour variations (ΔE) of all specimens were measured at baseline, after 1 week, and after 12 weeks of staining. Following the staining period, the specimens underwent a rinsing process using distilled water, were dried using a paper towel, and then subjected to colour evaluation from both sides.

Table 1. The utilised CAD/CAM materials.

Material (shade)	Manufacturer	Composition [□] (wt%)
IPS e-max CAD (HT,A2)	Ivoclar Vivadent AG, Schaan Liechtenstein	Silicon dioxide 57–80%, Lithium oxide 11–19%, Potassium oxide 0–13%, Phosphorus oxide 0–11% and other oxides
Cerasmart 270 (LT,A2)	GC Corp, Tokyo, Japan	Bis-MEPP, UDMA, dimethacrylate, Silica (20 nm), barium glass (300 nm) 71 wt%
Celtra Duo (LT,A2)	Dentsply Sirona, Germany	Zirconium-oxide 10.1%, Silicon dioxide 58%, Lithium oxide 18.5%, Phosphorus pentoxide 5%, Alumina 1.9%
Enamic (translucent)	VITA Zahnfabrik, Bad Säckingen, Germany	UDMA, TEGDMA, glass ceramic 86 wt%
Brilliant Crios (LT,A3)	Coltene, Switzerland	Bis-GMA, Bis-EMA, TEGDMA. 71 wt% barium glass
SFRC CAD (translucent)	Experimental, Stick Tech-GC member, Finland	UDMA, TEGDMA, Short glass fibre (200–300 μm & $\varnothing 7 \mu\text{m}$), Barium glass 77 wt%

[□] Composition based on manufacturer details.

TEGDMA: triethylene glycol dimethacrylate; UDMA: urethane dimethacrylate; Bis-MEPP: Bis (p-methacryloxy (ethoxy)1-2 phenyl)-propane; Bis-GMA: bisphenol-A-glycidyl dimethacrylate; Bis-EMA: Ethoxylated bisphenol-A-dimethacrylate; wt%: weight percentage.

The spectrophotometer Konica Minolta VLTCM-700d (Tokyo, Japan) was utilised to measure spectral reflectance and colour at baseline, and after staining. The measurements were conducted using the CIE Lab colour scale. The spectrophotometer utilised an aperture with a diameter of 3 mm and black background. The lighting and viewing setup adhered to the CIE diffuse/80 geometry, incorporating the specular component (SCI) geometry.

In order to determine the colour difference (ΔE), the average values of ΔL , Δa , and Δb for each specimen were employed in the subsequent formula:

$$\Delta E = [(\Delta L^*)^2 + (\Delta a^*)^2 + (\Delta b^*)^2]^{1/2}$$

Where variables ΔL , Δa , and Δb represent the variations in the L^* , a^* , and b^* values respectively, between the baseline and after staining.

The variable L^* indicates the lightness of the colour, ranging from black to white. The variable a^* provides information on the colour's position on the green and red axis, while b^* represents its position on the yellow and blue axis.

According to earlier research [18, 20, 21], a noticeable alteration in colour with a ΔE value greater than 1 will be considered acceptable, as long as it does not exceed $\Delta E = 3.3$.

The statistical studies were conducted using IBM Statistical Package for the Social Sciences (SPSS) Statistics software v28.0. The distribution of variance was tested using Levene's test of equality. In order to evaluate the differences in colour variation values among the specimens examined in various beverages and using different polishing techniques and immersion times, a 3-way analysis of variance (ANOVA) within each staining solution was conducted including factor interaction at a significance level of $\alpha = 0.05$. Subsequently, Tukey's multiple comparisons was conducted as a post hoc test to assess and evaluate the response of each material to staining solutions.

Results

Figures 1–4 illustrate the mean colour changes of specimens after 1 and 12 weeks of storage in various staining solutions, following either hand polishing or machine polishing. The material type and staining solution notably influenced the colour stability of the specimens. In each staining solution, material type, immersion time, and polishing technique demonstrated a significant effect on ΔE values ($p < 0.05$), with the exception of water and coke, where the polishing technique showed no significant effect ($p > 0.05$). Significant interaction between material type and immersion time was observed in specimens immersed in coke ($p < 0.05$).

The average ΔE values for specimens submerged in wine were determined to be substantially greater compared to the other beverages. Overall, IPS e.max exhibited the lowest ΔE values among all the tested CAD/CAM materials; however, this difference was not statistically significant ($p > 0.05$). SFRC CAD, Cerasmart 270, and Enamic displayed the highest ΔE values in wine ($p < 0.05$), indicating clinical unacceptability colour change ($\Delta E \geq 3.3$). On the other hand, Celtra demonstrated the highest

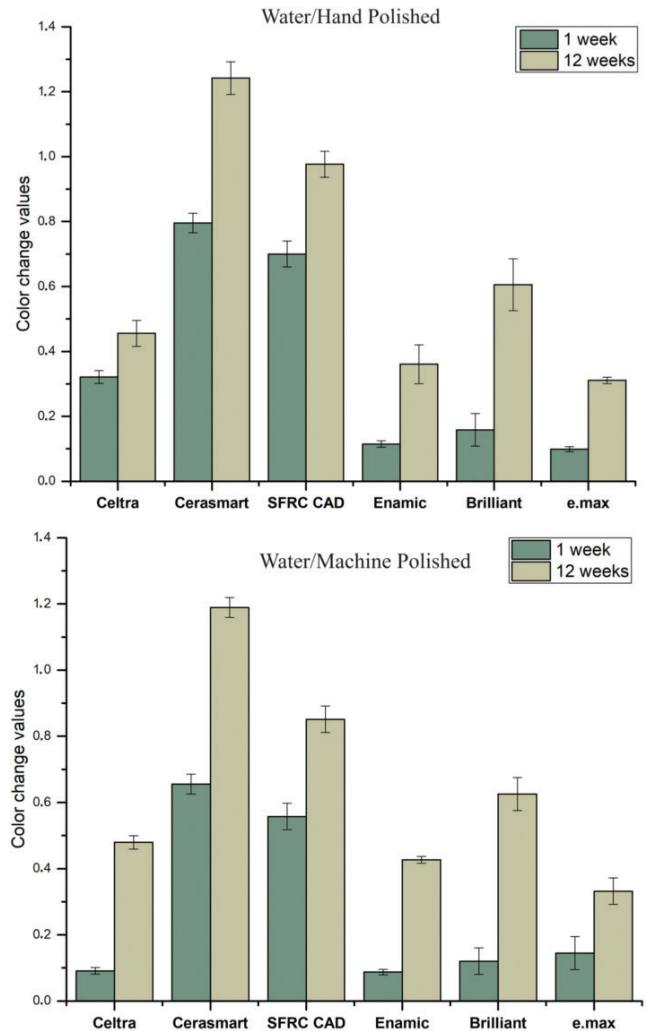


Figure 1. The mean colour change (ΔE) values of the CAD/CAM materials measured after 1 and 12 weeks of immersion in water, considering both hand and machine polishing techniques. Polishing technique showed no significant effect ($p > 0.05$).

ΔE values following immersion in coke for 12 weeks ($p < 0.05$). The impact of polishing technique (hand or machine) on staining was determined to be reliant upon the specific material and staining solution employed. The utilisation of machine polishing on IPS e.max, Enamic, and SFRC CAD specimens immersed in coffee and wine resulted in notably lower ΔE values ($p < 0.05$) when compared to the hand polishing technique. Conversely, no variations were noted for other materials exposed to various staining solutions.

Discussion

The colour stability of CAD/CAM restorations during use could be affected by the intake of diverse foods and beverages with varying pH levels, potentially causing staining and, maybe esthetic failure of the restorations [22]. This often requires replacing restorations in the aesthetic zones [23]. The phenomenon of discolouration poses a significant challenge for both patients and dentists, demanding more time and resources for retreatment.

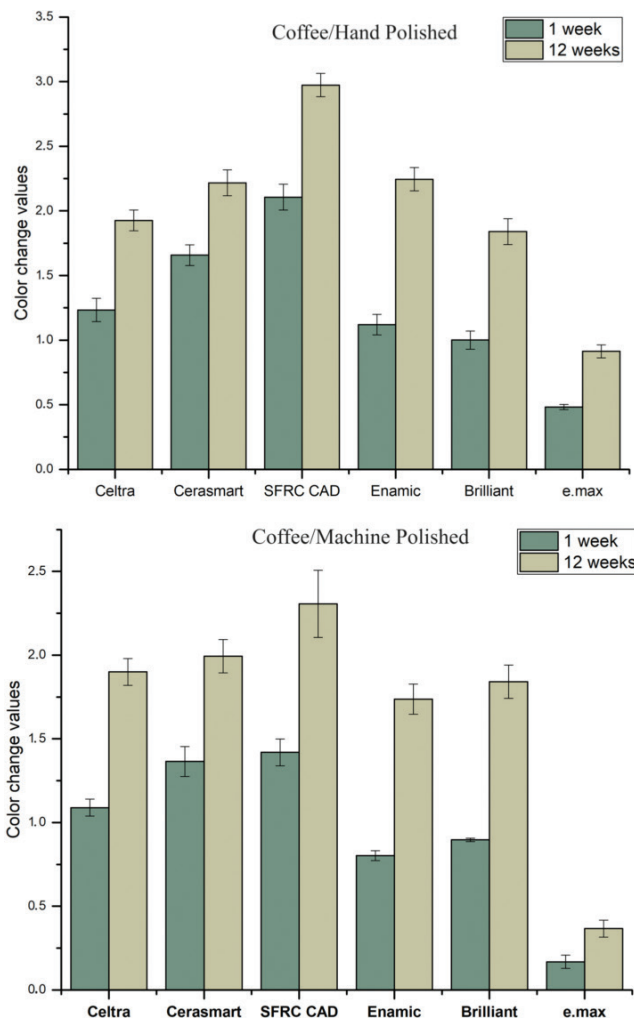


Figure 2. The mean colour change (ΔE) values of the CAD/CAM materials measured after 1 and 12 weeks of immersion in coffee, considering both hand and machine polishing techniques.

In this laboratory-based investigation, the impact of staining solutions, immersion time, and polishing techniques on the colour stability of six distinct CAD/CAM materials were assessed, revealing statistically significant differences. The findings led to the rejection of the null hypotheses, suggesting that the colour stability of CAD/CAM restorative materials differed considerably based on the staining solution type, materials used, immersion time, and the polishing technique applied.

Based on our results, SFRC CAD revealed comparable ΔE values compared to tested composite-based CAD/CAM materials. Thereby, microfibre filler loading had no negative impact on the colour stability of the SFRC CAD. This finding aligns with prior research that showed favourable surface and optical properties of SFRC CAD when compared to various particulate-filled composites [11, 14, 16]. Within the mentioned research, the microfibrils of the SFRC CAD did not protrude from surface after polishing or wear test; instead, they were polished in the resin matrix, resulting in often a uniformly smooth surface. Our results align with the study conducted by Uctasli et al., where flowable SFRC (everX Flow) demonstrated colour stability comparable to other conventional particulate-filled composites

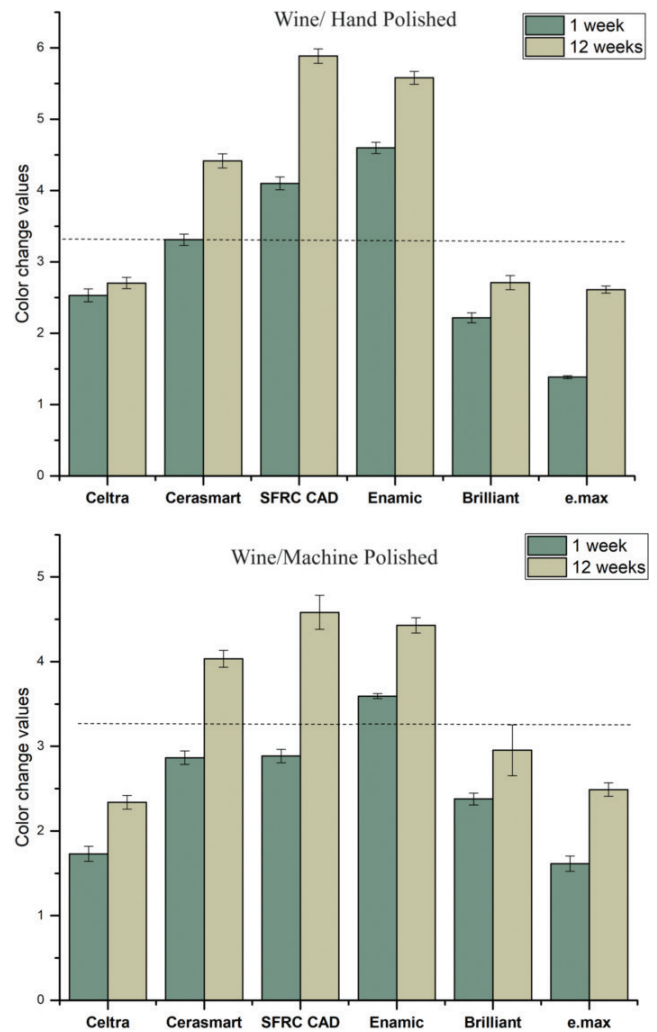


Figure 3. The mean colour change (ΔE) values of the CAD/CAM materials measured after 1 and 12 weeks of immersion in red wine, considering both hand and machine polishing techniques. Values that are higher than the dotted line suggest clinical unacceptability, with a threshold of $\Delta E \geq 3.3$.

that were tested [18]. These results give an indication that SFRC CAD has the potential to be utilised safely as monolithic restorations across a wider variety of clinical scenarios.

Generally, the colour stability of composite-based or hybrid CAD/CAM materials was inferior in comparison to glass-ceramic materials. The staining susceptibility of CAD/CAM composites can be affected by different parameters, including the extent of water absorption and the hydrophilicity of the composite matrix [24]. If a composite material is hydrophilic, it is also susceptible to absorbing various fluids, which might lead to discolouration. The diverse compositions of composites result in variations in their sensitivity to staining, principally due to their water absorption characteristics. Water is thought to act as a channel for stains to enter the composite matrix [25]. The particulate fillers in CAD/CAM composites do not take in water throughout the material, although they can absorb water on their surface. A higher amount of resin matrix in the composites results in higher water absorption and diminished bonding between the resin matrix and filler particles. Swelling and plasticising actions can cause the production of microcracks in the composite matrix,

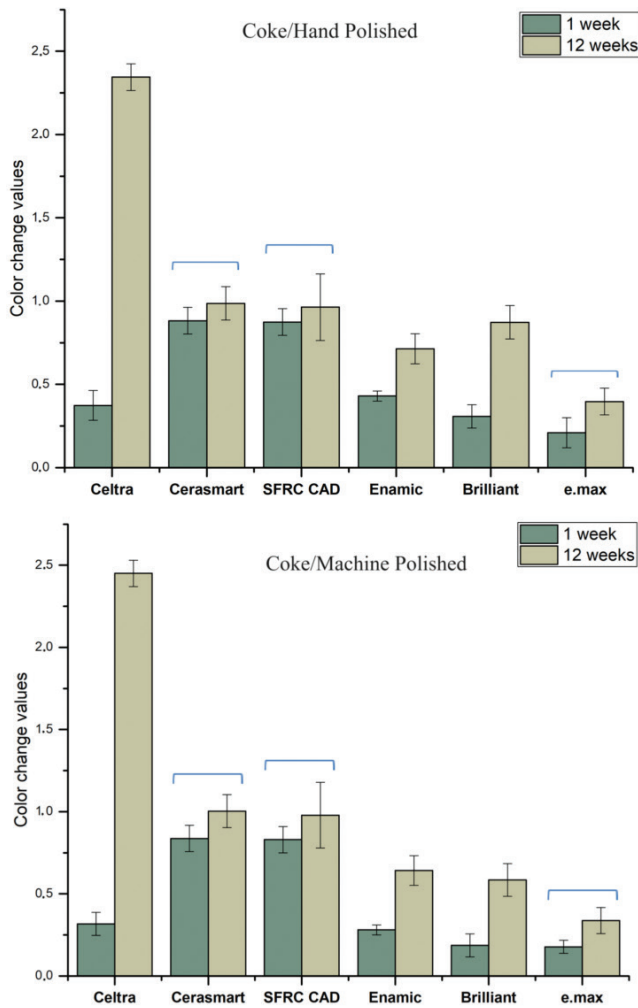


Figure 4. The mean colour change (ΔE) values of the CAD/CAM materials measured after 1 and 12 weeks of immersion in coke, considering both hand and machine polishing techniques. Polishing technique showed no significant effect ($p > 0.05$) and groups joined by a line are not significantly difference.

along with the development of gaps between the filler and matrix. These conditions promote the entry of stains and the resulting colour change of the restorations [25].

It is well acknowledged that glass-ceramic CAD/CAM materials have better colour stability than composite-based CAD/CAM materials [26]. This is in line with our results, as IPS e.max showed better colour stability than composite-based CAD/CAM materials. While Celtra is a glass-ceramic material, its colour stability was found to be lower than that of IPS e.max. The colour stability of glass-ceramic materials can be influenced by several parameters, such as the crystalline structure, grain size, and porosity [22].

Discolouration can be evaluated by either visual or instrumental methods. We utilised spectrophotometry in our investigation, a method that eliminates any subjective interpretation when doing visual colour comparisons. The reliability of spectrophotometry as a tool in dental materials studies has been acknowledged [18, 27]. The ΔE value quantifies the extent of colour changes that an observer may see in the

materials either after immersion or over a period of time. Thus, ΔE is a more significant measure than the separate ΔL , Δa , and Δb values [28].

It is crucial to note that within dental research, two colour difference formulas have been utilised extensively over the years [29]. Recent research has indicated that the CIEDE2000 colour difference formula, compared to the CIE LAB formula utilised in our study, offers a superior fit when assessing visual tolerances [29–32]. The CIEDE2000 formula is believed to more accurately reflect human perception of colour differences, with a reported 95% agreement with visual observations, compared to the 75% agreement of the CIE LAB formula [30, 31]. However, CIE LAB formula remains applicable and valid for calculating colour or translucency differences across materials [32].

We evaluated the colour stability of CAD/CAM materials by submerging them in four frequently consumed beverages (water, coffee, red wine, and coke) over a period of 12 weeks. In order to mimic real patterns of beverage consumption, we took into account the mean duration for consuming a cup of coffee as an example, which is roughly 15 min. Furthermore, taking into account the typical coffee intake of three cups per day among consumers of coffee, our 12-week immersion period accurately replicated the experience of consuming the beverage for a duration of 7 years [33].

Our investigation validated prior research findings [34, 35] that red wine causes the most noticeable discolouration of CAD/CAM materials, which is easily visible without the need for a high level of inspection. The discolouration caused by coffee and wine can be explained by the absorption of their pigments into the organic component of the composites [33]. Remarkably, coke containing phosphoric and citric acids, with a pH of around 2.5, did not exhibit a significant correlation with changes in colour in CAD/CAM materials when compared to coffee and wine. Acids can exhibit different behaviours in terms of facilitating dissolution, absorption of water, and erosion of materials. Bagheri et al. and Ertas et al. have proposed that the lack of yellow colourants in coke leads to reduced discolouration compared to the staining induced by coffee and wine [25, 36]. In addition, numerous studies have demonstrated that, despite their acidic nature, carbonated beverages like coke cause only modest discolouration of CAD/CAM materials when compared to other dark beverages [26, 35].

According to Paravina and his colleagues, the colour difference threshold for teeth and tooth-coloured restorations was noted to be 2.7 when utilising the CIE LAB formula [30]. However, various other studies have reported divergent values, a difference attributed to variations in the number and types of observers, research locations, and the colour difference formulas employed [32]. Multiple investigations have indicated that ΔE values ranging from 1 to 3 can be detected by the eye alone; however, ΔE levels beyond 3.3 are thought to be clinically unacceptable [18, 20, 21]. Based on these principles, the CAD/CAM materials examined in this work showed satisfactory colour stability when subjected to staining solutions for a

duration of 12 weeks, except when exposed to wine. Among the tested materials, only SFRC CAD, Cerasmart 270, and Enamic in wine exhibited colour change values surpassing 3.3 (Figure 3). The inclusion of UDMA in the structure of these CAD/CAM materials (Table 1) may explain this behaviour. These materials are prone to releasing monomers in acidic conditions more than Brilliant, which is formulated with Bis-GMA and Bis-EMA resin.

The differences in colour stability reported among the investigated composite-based CAD/CAM materials might also be related to the variations in filler/resin ratio (Table 1). Furthermore, the colour change that was noticed might also be linked to the utilisation of the silane agent. The discolouration caused by silanisation of inorganic particles is attributed to the silane's high water sorption capacity [37]. Moreover, the shade of the material is an additional factor that affects CAD/CAM composite staining. The inclusion of pigments in darker colours typically enhances their ability to achieve accurate colour matching. Consequently, translucent shades, which do not include these pigments, may undergo a more pronounced level of colour change [38].

The literature has identified polishing methods as a potential element that can impact colour stability. Nevertheless, there is a lack of agreement regarding the influence of surface treatment on the change of colour caused by staining. Conflicting reports exist about the results of different polishing methods [39–42]. Several research proposes that the level of smoothness in a surface does not always result in higher resistance to staining. Conversely, other studies indicate that the lack of appropriate polishing can make specimens more prone to staining. The current research on the correlation between surface treatment and colour stability remains unclear, necessitating additional investigation to provide clarity on this issue. For this investigation, the Sof-Lex™ Polishing System was used to polish one surface of all the CAD/CAM specimens, aiming at accurately imitating practical situations in clinical settings. The opposite side of the specimens was subjected to a precise laboratory method including 4000-grit polishing, resulting in a highly polished surface. Surprisingly, the results demonstrated that the polishing procedure did not exert a notable influence on the colour change of the composite specimens across all CAD/CAM materials. This result aligns with the investigation conducted by Imamura et al., which also demonstrated that the polishing technique had a restricted influence on the discolouration of composites [37]. It is also in line with the research conducted by Sasany et al., who illustrated the successful use of the Sof-Lex™ polishing system for chair-side CAD/CAM material polishing [40].

Research evaluating colour stability *in vitro* has inherent methodological limitations. The aim of this study was to mimic the prolonged impact of oral environmental factors within a condensed 12-week timeframe, with the goal of predicting the colour stability of the SFRC CAD material. It is crucial to acknowledge that in the oral environment, elements such as heating from food and drink, saliva, and other fluids can exert a more substantial impact. In addition, chewing can modify the

texture of the composite material, resulting in the retention of deposits and elements that cause discolouration on uneven surfaces for extended durations.

Conclusions

The following conclusions can be drawn, given the limitations of the present study:

1. The colour stability of tested SFRC CAD, was comparable to other composite-based CAD/CAM materials.
2. The extent of colour change was influenced by the staining solution, immersion time, polishing technique, and the specific material used.
3. Among all of the tested CAD/CAM materials, IPS e.max showed the highest level of colour stability.

Declarations

Ethics approval and consent to participate

Not applicable.

Consent for publication

Not applicable.

Availability of data and materials

The datasets used and/or analysed during the current study available from the corresponding author on reasonable request.

Conflicts of Interests

Author P.V. consults for Stick Tech – Member of the GC Group in R&D and training. Other authors declare to have no conflict of interests.

Funding

The authors declared that this study has received no financial support.

Authors' contributions

Study design, L.L. and S.G.; collection of data, S.G.; and U.M.B. and K.W.; data analysis/interpretation, S.G., U.M.B. and L.L.; writing-original draft preparation, S.G.; writing-review and editing, U.M.B, L.L. and P.V.

Acknowledgments

This study belongs to the research activity of BioCity Turku Biomaterials Research Program (www.biomaterials.utu.fi).

References

- [1] Sampaio FBWR, Özcan M, Gimenez TC, Moreira MSNA, Tedesco TK, Morimoto S. Effects of manufacturing methods on the survival rate of ceramic and indirect composite restorations: a systematic review and meta-analysis. *J Esthet Restor Dent*. 2019;31:561–571. <https://doi.org/10.1111/jerd.12555>
- [2] Spitznagel FA, Boldt J, Gierthmuehlen PC. CAD/CAM ceramic restorative materials for natural teeth. *J Dent Res*. 2018;97:1082–1091. <https://doi.org/10.1177/0022034518779759>
- [3] Skorulska A, Piszko P, Rybak Z, Szymonowicz M, Dobrzyński M. Review on polymer, ceramic and composite materials for CAD/CAM indirect restorations in dentistry-application, mechanical characteristics and comparison. *Materials (Basel)*. 2021;14:1592. <https://doi.org/10.3390/ma14071592>
- [4] Becker M, Chaar MS, Garling A, Kern M. Fifteen-year outcome of posterior all-ceramic inlay-retained fixed dental prostheses. *J Dent*. 2019;89:103174. <https://doi.org/10.1016/j.jdent.2019.07.012>
- [5] González-Angulo E, Fernández-Estevan L, Casas-Terrón J, Senent-Vicente G, Fons-Badal C, García-Sala Bonmatí F, et al. Microtensile bond strength of CAD-CAM restorative dental material blocks to resin cement: an in vitro study. *Materials (Basel)*. 2023;16:4796. <https://doi.org/10.3390/ma16134796>
- [6] Özcan M, Bernasconi M. Adhesion to zirconia used for dental restorations: a systematic review and meta-analysis. *J Adhes Dent*. 2015;17:7–26.
- [7] Abdulmajeed A, Sulaiman T, Abdulmajeed A, Bencharit S, Närhi T. Fracture load of different Zirconia types: a mastication simulation study. *J Prosthodont*. 2020 Dec;29(9):787–791. <https://doi.org/10.1111/jopr.13242>
- [8] Peskersoy C, Sahan HM. Finite element analysis and nanomechanical properties of composite and ceramic dental onlays. *Comput Methods Biomech Biomed Engin*. 2022;25:1649–1661. <https://doi.org/10.1080/10255842.2022.2032004>
- [9] Saratti CM, Rocca GT, Durual S, Lohbauer U, Ferracane JL, Scherrer SS. Fractography of clinical failures of indirect resin composite endocrown and overlay restorations. *Dent Mater*. 2021 Jun;37(6):e341–e359. <https://doi.org/10.1016/j.dental.2021.02.002>
- [10] Tsitrou EA, Northeast SE, van Noort R. Brittleness index of machinable dental materials and its relation to the marginal chipping factor. *J Dent*. 2007 Dec;35(12):897–902. <https://doi.org/10.1016/j.jdent.2007.07.002>
- [11] Lassila L, Novotny R, Säilynoja E, Vallittu PK, Garoushi S. Wear behavior at margins of direct composite with CAD/CAM composite and enamel. *Clin Oral Investig*. 2023 May;27(5):2419–2426. <https://doi.org/10.1007/s00784-023-04883-w>
- [12] Belli R, Wendler M, de Ligny D, Cicconi MR, Petschelt A, Peterlik H, et al. Chairside CAD/CAM materials. Part 1: measurement of elastic constants and microstructural characterization. *Dent Mater*. 2017 Jan;33(1):84–98. <https://doi.org/10.1016/j.dental.2016.10.009>
- [13] Lassila L, Mangoush E, Vallittu PK, Garoushi S. Fracture behavior of discontinuous fiber-reinforced composite inlay-retained fixed partial denture before and after fatigue aging. *J Prosthodont Res*. 2023 Apr 12;67(2):271–277. https://doi.org/10.2186/jpr.JPR_D_22_00050
- [14] Mangoush E, Lassila L, Vallittu PK, Garoushi S. Microstructure and surface characteristics of short-fiber reinforced CAD/CAM composite blocks. *Eur J Prosthodont Restor Dent*. 2021 Aug 31;29(3): 166–174. <https://doi.org/10.1111/eos.12815>
- [15] Mangoush E, Garoushi S, Vallittu PK, Lassila L. Influence of short fiber-reinforced composites on fracture resistance of single-structure restorations. *Eur J Prosthodont Restor Dent*. 2020 Nov 30;28(4):189–198.
- [16] Mangoush E, Lassila L, Vallittu PK, Garoushi S. Shear-bond strength and optical properties of short fiber-reinforced CAD/CAM composite blocks. *Eur J Oral Sci*. 2021 Oct;129(5):e12815. <https://doi.org/10.1111/eos.12815>
- [17] Mangoush E, Garoushi S, Vallittu P, Lassila L. Load-bearing capacity and wear characteristics of short fiber-reinforced composite and glass ceramic fixed partial dentures. *Eur J Oral Sci*. 2023 Oct-Nov;131(5–6):e12951. <https://doi.org/10.1111/eos.12951>
- [18] Uctasli MB, Garoushi S, Uctasli M, Vallittu PK, Lassila L. A comparative assessment of color stability among various commercial resin composites. *BMC Oral Health*. 2023 Oct 24;23(1):789. <https://doi.org/10.1186/s12903-023-03515-9>
- [19] Choi JW, Lee MJ, Oh SH, Kim KM. Changes in the physical properties and color stability of aesthetic restorative materials caused by various beverages. *Dent Mater J*. 2019 Feb 8;38(1):33–40. <https://doi.org/10.4012/dmj.2017-247>
- [20] Villalta P, Lu H, Okte Z, Garcia-Godoy F, Powers JM. Effects of staining and bleaching on color change of dental composite resins. *J Prosthet Dent*. 2006 Feb;95(2):137–142. <https://doi.org/10.1016/j.prosdent.2005.11.019>
- [21] Yilmaz B, Karaagaciloglu L. In vitro evaluation of color replication of metal ceramic specimens using visual and instrumental color determinations. *J Prosthet Dent*. 2011 Jan;105(1):21–27. [https://doi.org/10.1016/S0022-3913\(10\)60185-0](https://doi.org/10.1016/S0022-3913(10)60185-0)
- [22] Choi SH, Shim HW, Lee HH, Ahn JS, Kim YJ, Shin SY, et al. Effects of ultraviolet weathering aging on the color stability and biocompatibility of various computer-aided design and computer-aided manufacturing glass-ceramic materials. *J Dent*. 2023 Dec;139:104746. <https://doi.org/10.1016/j.jdent.2023.104746>
- [23] Rauch A, Lorenz L, Reich S, Hahnel S, Schmutzler A, Schierz O. Long-term survival of monolithic tooth-supported lithium disilicate crowns fabricated using a chairside approach: 15-year results. *Clin Oral Investig*. 2023 Jul;27(7):3983–3989. <https://doi.org/10.1007/s00784-023-05023-0>
- [24] Sulaiman TA, Suliman AA, Mohamed EA, Rodgers B, Altak A, Johnston WM. Optical properties of bisacryl-, composite-, ceramic- resin restorative materials: an aging simulation study. *J Esthet Restor Dent*. 2021 Sep;33(6):913–918.
- [25] Bagheri R, Burrow MF, Tyas M. Influence of food-simulating solutions and surface finish on susceptibility to staining of aesthetic restorative materials. *J Dent*. 2005;33:389–398. <https://doi.org/10.1016/j.jdent.2004.10.018>
- [26] Eldwakhly E, Ahmed DRM, Soliman M, Abbas MM, Badrawy W. Color and translucency stability of novel restorative CAD/CAM materials. *Dent Med Probl*. 2019 Oct-Dec;56(4):349–356.
- [27] He J, Garoushi S, Säilynoja E, Vallittu P, Lassila L. Surface integrity of dimethacrylate composite resins with low shrinkage comonomers. *Materials (Basel)*. 2021 Mar 26;14(7):1614. <https://doi.org/10.3390/ma14071614>
- [28] Yannikakis SA, Zissis AJ, Polyzois GL, Caroni C. Colour stability of provisional resin restorative materials. *J Prosthet Dent*. 1998;80:533–539.
- [29] Gómez-Polo C, Portillo Muñoz M, Lorenzo Luengo MC, Vicente P, Galindo P, Martín Casado AM. Comparison of the CIELab and CIEDE2000 color difference formulas. *J Prosthet Dent*. 2016 Jan;115(1):65–70. <https://doi.org/10.1016/j.prosdent.2015.07.001>
- [30] Paravina RD, Ghinea R, Herrera LJ, Bona AD, Iglie C, Linninger M, et al. Color difference thresholds in dentistry. *J Esthet Restor Dent*. 2015 Mar-Apr;27 Suppl 1:S1–S9. <https://doi.org/10.1111/jerd.12149>
- [31] Ghinea R, Pérez MM, Herrera LJ, Rivas MJ, Yebra A, Paravina RD. Color difference thresholds in dental ceramics. *J Dent*. 2010;38 Suppl 2:e57–e64. <https://doi.org/10.1016/j.jdent.2010.07.008>
- [32] Paravina RD, Pérez MM, Ghinea R. Acceptability and perceptibility thresholds in dentistry: a comprehensive review of clinical and research applications. *J Esthet Restor Dent*. 2019 Mar;31(2):103–112. <https://doi.org/10.1111/jerd.12465>
- [33] Guler AU, Yilmaz F, Kulunk T, Guler E, Kurt S. Effects of different drinks on stainability of resin composite provisional restorative materials. *J Prosthet Dent*. 2005 Aug;94(2):118–124.

- [34] Kurklu ZGB, Sonkaya E. Comparison of discoloration of ceramic containing 3D printable material and CAD/CAM blocks. *Dent Mater J.* 2024; 43(1):28-35. <https://doi.org/10.4012/dmj.2023-131>
- [35] Aydın N, Karaoğlanoğlu S, Oktay EA, Kılıçarslan MA. Investigating the color changes on resin-based CAD/CAM Blocks. *J Esthet Restor Dent.* 2020 Mar;32(2):251–256.
- [36] Ertaş E, Güler AU, Yücel AC, Köprülü H, Güler E. Color stability of resin composites after immersion in different drinks. *Mater J.* 2006;25:371–376. <https://doi.org/10.4012/dmj.25.371>
- [37] Imamura S, Takahashi H, Hayakawa I, Loyaga-Rendon PG, Minakuchi S. Effect of filler type and polishing on the discoloration of composite resin artificial teeth. *Dent Mater J.* 2008 Nov;27(6):802–808. <https://doi.org/10.4012/dmj.27.802>
- [38] Arregui M, Giner L, Ferrari M, Vallés M, Mercadé M. Six-month color change and water sorption of 9 new-generation flowable composites in 6 staining solutions. *Braz Oral Res.* 2016 Nov 28;30(1):e123. <https://doi.org/10.1590/1807-3107bor-2016.vol30.0123>
- [39] Brito MG, Amaral FL, Turssi CP, Hofling RT, França FM. Effect of chemical or mechanical finishing/polishing and immersion in staining solutions on the roughness, microhardness, and color stability of CAD-CAM monolithic ceramics. *Acta Odontol Latinoam.* 2023 Aug 31;36(2):86–95. <https://doi.org/10.54589/aol.36/2/86>
- [40] Sasany R, Ergün Kunt G, Koca MF. Influence different polishing systems on roughness and colour stability of chairside CAD/CAM blocks with laminate veneer thickness. *J Appl Biomater Funct Mater.* 2022 Jan-Dec;20:22808000221086493. <https://doi.org/10.1177/22808000221086493>
- [41] Stawarczyk B, Sener B, Trottmann A, Roos M, Ozcan M, Hämmerle CH. Discoloration of manually fabricated resins and industrially fabricated CAD/CAM blocks versus glass-ceramic: effect of storage media, duration, and subsequent polishing. *Dent Mater J.* 2012;31(3):377–383. <https://doi.org/10.4012/dmj.2011-238>
- [42] Kilinc H, Turgut S. Optical behaviors of esthetic CAD-CAM restorations after different surface finishing and polishing procedures and UV aging: an in vitro study. *J Prosthet Dent.* 2018 Jul;120(1):107–113. <https://doi.org/10.1016/j.prosdent.2017.09.019>